

# 5-Part-Diff Auto Hematology Analyzer

Mode:Whole Blood+Auto+CD

Serial No.:220

BarCode:

Name:

Sex:

Case ID:

Patient Type:

Age:

Group:General

Department:

Blood:

Bed ID:


Diagnose:

Test Time:2017-05-17 19:44:59

Remark:

Print Time:2017-09-06 11:25:31

Item	Result	Unit	Range	Hit
<b>WBC (WBC)</b>	6.54	10 <sup>9</sup> /L	10.00 ~ 4.00	
LYM% (LYM%)	3.89	%	40.00 ~ 20.00	L
MON% (MON%)	6.01	%	10.00 ~ 3.00	
<b>NEU% (NEU%)</b>	<b>89.46</b>	<b>%</b>	<b>70.00 ~ 50.00</b>	<b>H</b>
EOS% (EOS%)	0.60	%	5.00 ~ 0.50	
BASO% (BASO%)	0.04	%	1.00 ~ 0.00	
LYM# (LYM#)	0.254	10 <sup>9</sup> /L	4.000 ~ 0.800	L
MON# (MON#)	0.393	10 <sup>9</sup> /L	1.200 ~ 0.120	
NEU# (NEU#)	5.851	10 <sup>9</sup> /L	7.000 ~ 2.000	
EOS# (EOS#)	0.039	10 <sup>9</sup> /L	0.500 ~ 0.020	
BASO# (BASO#)	0.003	10 <sup>9</sup> /L	0.100 ~ 0.000	
<b>RBC (RBC)</b>	2.65	10 <sup>12</sup> /L	5.50 ~ 3.50	L
<b>HGB (HGB)</b>	89	g/L	160 ~ 110	L
HCT (HCT)	20.4	%	54.0 ~ 37.0	L
MCV (MCV)	77.1	fL	100.0 ~ 80.0	L
MCH (MCH)	33.5	pg	34.0 ~ 27.0	
<b>MCHC (MCHC)</b>	<b>436</b>	<b>g/L</b>	<b>360 ~ 320</b>	<b>H</b>
<b>RDW_SD (RDW_SD)</b>	<b>77.0</b>	<b>fL</b>	<b>56.0 ~ 35.0</b>	<b>H</b>
RDW_CV (RDW_CV)	14.7	%	16.0 ~ 11.0	
<b>PLT (PLT)</b>	11	10 <sup>9</sup> /L	300 ~ 100	L
MPV (MPV)	3.9	fL	12.0 ~ 6.5	L
PDW (PDW)	2.8	fL	17.0 ~ 9.0	L
PCT (PCT)	0.00	%	0.28 ~ 0.11	L
P_LCR (P_LCR)	35.32	%	45.00 ~ 9.00	
P_LCC (P_LCC)	4	10 <sup>9</sup> /L	129 ~ 13	L

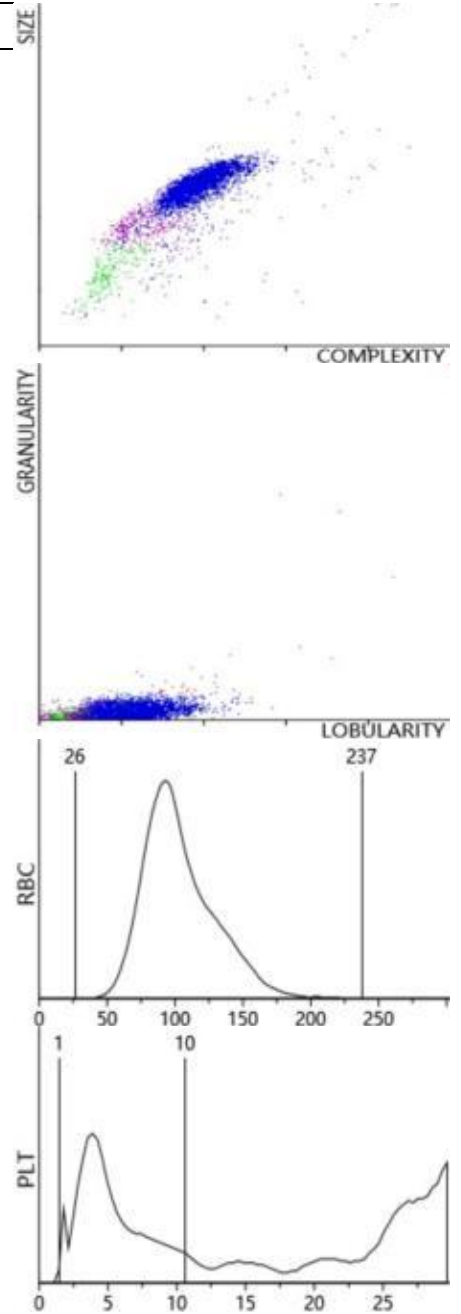

Sender:

Operator:admin

Auditor:

\*This result is valid only for current sample\*